




# For Adult (≥18 years) Non-Traumatic Cardiac Arrest Maximum Patient Weight 300 lbs.

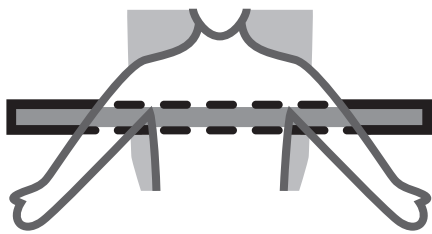

- Remove ALL clothing from torso (both front and back) to ensure skin-to-platform contact
- Align armpits onto yellow line on Platform

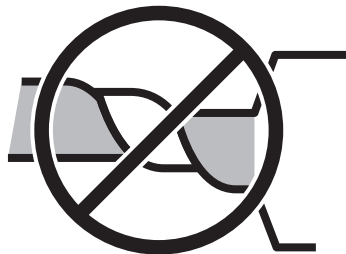


Do not twist the chest bands

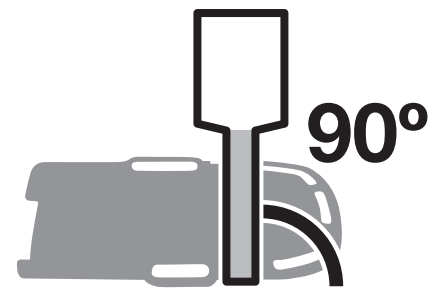

Maintain chest bands at 90 degrees to Platform and free of obstructions

1. Power up AutoPulse

2. Close chest bands

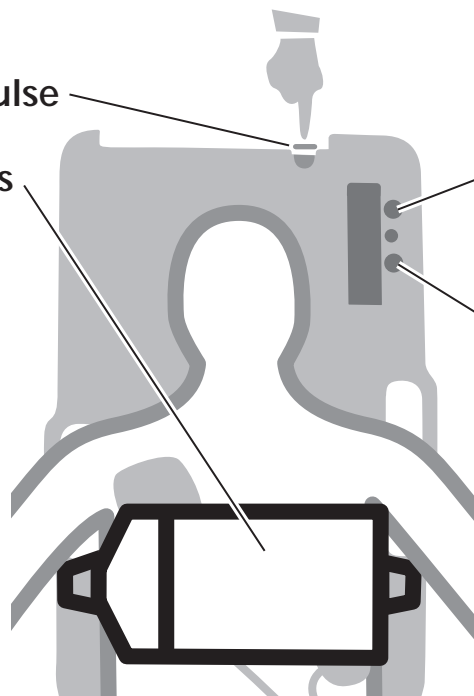

3. Press CONTINUE (green button)

4. Press START (green button) to begin compressions

To pause or stop operation press STOP (orange button)


Follow all local protocols and procedures.

Review User Guides and complete in-service training.

## Troubleshooting

### For Fault/User Advisory

- Lift up and fully extend both chest bands.
- Check both lateral and vertical patient alignment.
- Verify that chest bands are not twisted, are 90 degrees to the Platform and are free of obstructions.
- Press **RESTART** (green button) and follow on-screen instructions to begin compressions.

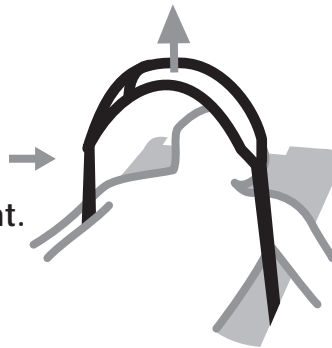

If you cannot rectify problem immediately open chest bands and revert to manual CPR.

